



Insect-inspired acoustic micro-sensors

Y Zhang, A Reid and JFC Windmill

Micro-Electro Mechanical System (MEMS) microphones inspired by the remarkable phonotactic capability of *Ormia ochracea* offer the promise of microscale directional microphones with a greatly reduced need for post-processing of signals. Gravid *O. ochracea* females can locate their host cricket's 5 kHz mating calls to an accuracy of less than 2° despite having a distance of approximately 500 μm between the ears. MEMS devices based on the principles of operation of *O. ochracea*'s hearing system have been well studied, however commercial implementation has proven challenging due to the system's reliance on carefully tailored ratios of stiffness and damping, which are difficult to realize in standard MEMS fabrication processes, necessitating a trade-off between wide-band operation and sensitivity. A survey of the variety of strategies that have been followed to address these inherent challenges is presented.

Address

Centre for Ultrasonic Engineering, University of Strathclyde, 204 George Street, Glasgow, G1 1XW, United Kingdom

Corresponding author: Windmill, JFC (james.windmill@strath.ac.uk)

Current Opinion in Insect Science 2018, 30:33–38

This review comes from a themed issue on **Insect bio-inspired micro and nanotechnologies**

Edited by Jérôme Casas

<https://doi.org/10.1016/j.cois.2018.09.002>

2214-5745/© 2018 The Authors. Published by Elsevier Inc. This is an open access article under the CC BY license (<http://creativecommons.org/licenses/by/4.0/>).

Introduction

The traditional method of sound source localization is to build a microphone array which combines at least two independent omnidirectional microphones [1]. Calculating the incident angle of sound waves then depends on the separating distance (i.e. time delay) between the microphones receiving the plane waves [2–4]. Similar to microphone arrays, many large animals including human beings have two ears with sufficient separation that the nervous system is able to resolve the interaural time difference (ITD) and interaural intensity difference (IID) to determine the source location. The requirement for spatial separation poses a fundamental problem for sound localization in small animals [5] and in micro-scale devices (i.e. Micro-Electro-Mechanic-System (MEMS) devices) smaller than the wavelength of interest.

In the 1990's, *O. ochracea* was found to have a great capability for detecting sound source [6,7^{**},8]. The parasitic female *Ormia* uses auditory cues to localize the mating call of a host *Gryllus*, a genus of cricket, and then deposits its predaceous larvae on the host [9]. The cricket's mating call has a fundamental frequency around 5 kHz and wavelength at approximately 70 mm, compared to the interaural distance of *Ormia* that is only around 520 μm [10,11]. Despite the extremely small distance that gives the original maximum ITD and IID as approximately 1.5 μs and 1 dB [12], respectively, experimental investigations show that it can localize the mating call with a resolution less than 2° [13]. This high accuracy is attributed to the mechanical coupling structure of *Ormia*'s ear, as shown in Figure 1(a) and (b), which enhances both ITD and IID by up to 40 times greater than the original values at 5 kHz [14^{**}]. The first resonance is a rocking mode about the bridge centre point, and the second is a translational mode with each end of the bridge moving in-phase while the bridge bends in the middle as shown in Figure 1(c). The response of the *Ormia* ear at any frequency is then described by a linear combination of these resonance modes [15^{**}].


Ormia-inspired MEMS microphone designs can be broadly separated into two main categories in terms of their directivity: the first-order and the second-order. The response of the first-order microphones is proportional to the pressure gradient combined with the integral of pressure across the surface [16,17] while second-order microphones have directional responses that are proportional to the difference between the gradients [18].

First order *Ormia* inspired microphones

First-order *Ormia*-inspired microphone designs include the see-saw model [19–22] and the clamped diaphragms model [23–27] as shown in Figure 2. See-saw models' defining characteristic is a pivot between two unclamped diaphragms. An early iteration of this design from Miles *et al.* [19,28,29] used a polysilicon diaphragm supported with well-distributed crossed stiffeners [30^{*},31,32] to tailor the relative sensitivities of the rocking and translational modes of the device while lowering the overall mass. As with most of the designs, amplification of directional cues occurs only in a single narrow working frequency band [33–35].

The transduction method plays a key role in the sensitivity and the amplification of directional cues. Three transduction methods have been attempted by Miles *et al.*, paralleled-plate capacitive sensing [20,36], optical sensing [31,37,38^{*}], and comb-finger capacitive sensing


Figure 1

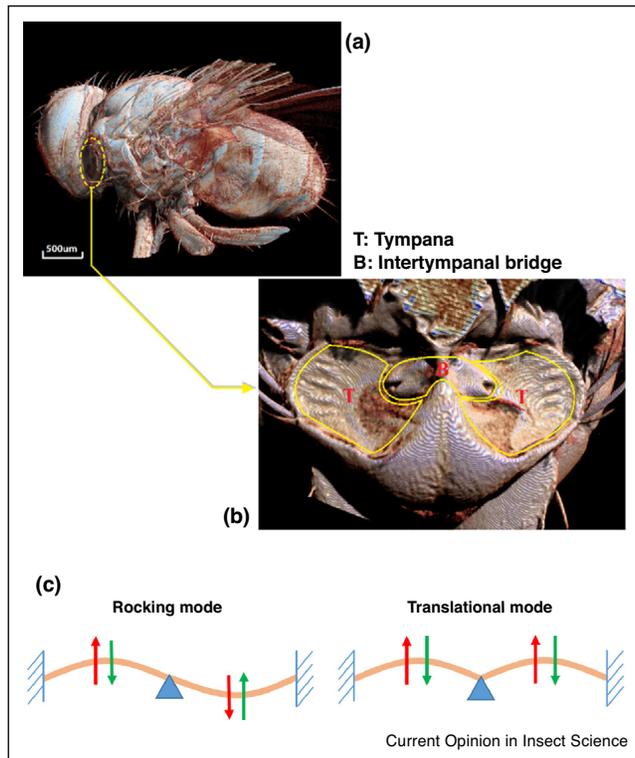

MicroCT scanned images of *Ormia ochracea*: (a) The side view of *Ormia*'s body. (b) The frontal face of the hearing organ. (c) A sketch of the two main resonance modes: rocking mode and translational mode.

[17,39°]. For parallel-plate sensing, the SNR is negatively influenced by electronic noise, and the viscous damping caused by the air between the diaphragm and the back-plate leads to thermal noise [40]. Optical sensing based on a phase-sensitive diffraction grating structure can lower noise and power requirements compared to capacitive sensing. This method is achieved by incorporating interdigitated comb fingers at the ends of the diaphragm. However, optical sensing is a comparably high-cost transduction method, which is generally considered not suitable for commercial use. Capacitive combs, in contrast, can be fabricated in a single layer MEMS device and offers the benefits of extremely low noise [41°,42] at the trade-off of electrical sensitivity. In recent years PZT

Figure 2

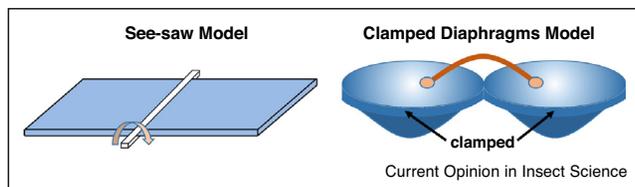


Schematic diaphragms of see-saw and clamped diaphragms *Ormia* inspired microphone models.

[43–45] or Aluminium Nitride [46] thin film layers have been used in combination with cantilevers connecting to the diaphragms to provide an alternative method of transduction.

The method of transduction has a particular impact for *Ormia*-inspired microphones due to the sensitivity of the desired amplification of ITD to damping. High damping ratios from capacitive back-plates and thin film damping broaden the frequency range of the increase in directional cues at the expense of the gain of amplification [47°], while lower damping ratios benefit from increased sensitivity but produce only a single narrow working band [48°]. Obtaining a flat amplification of ITD or IID across a usable frequency range, a critical element of hearing-aid applications, may be achieved by sacrificing significant gain in the amplification as demonstrated in two designs from Miles *et al.* — one using a capacitive comb sensing scheme [40] and the other an optical diffraction grating [49] — which nevertheless show the same mechanical characteristics. The resonance frequencies for these devices places the lower, rocking mode at 735 Hz with the higher, translational mode at 15 427 Hz. The estimated damping remains low, given the absence of a back-plate in either design, at 0.16 for the rocking mode and 0.25 for the translational mode with the result that the devices provide a flat gain of approximately 1.5 times the ITD. An alternative strategy was developed by Zhang *et al.* [50–53,54°,55°] where multiple working frequency bands extend the useable working range of the device. This extends the see-saw design pattern through the use of asymmetric diaphragms and an inner and outer diaphragm configuration, with each providing two frequency bands. The design used a piezoelectric sensing system, and produced directional responses at frequency bands below 10 kHz. Figure 3 shows the latest published development of the device.

Measuring amplifications in intensity difference poses additional challenges. Since the amplitude of response will be proportional to the local sound pressure a direct comparison would require the use of a reference, omnidirectional microphone. This enlarges the entire package size and brings errors caused by the offset between the *Ormia* inspired microphone and the omnidirectional one. Yu *et al.* circumvented this problem by taking the ratio of amplitudes of the two diaphragms [24,56,57] and their phase difference which were termed the mechanical Interaural Intensity Difference (mIID) and mechanical Interaural Phase Difference (mIPD) respectively. These measures obviate the need for a reference microphone, however as the motion of the diaphragm on the contralateral side to the source is ideally greatly suppressed the denominator of these equations is often near zero leading to a high Cauchy-like noise error in the measurement of sound angle. The devices developed by Yu *et al.* are intended to directly mimic the *Ormia* ear's single

Figure 3

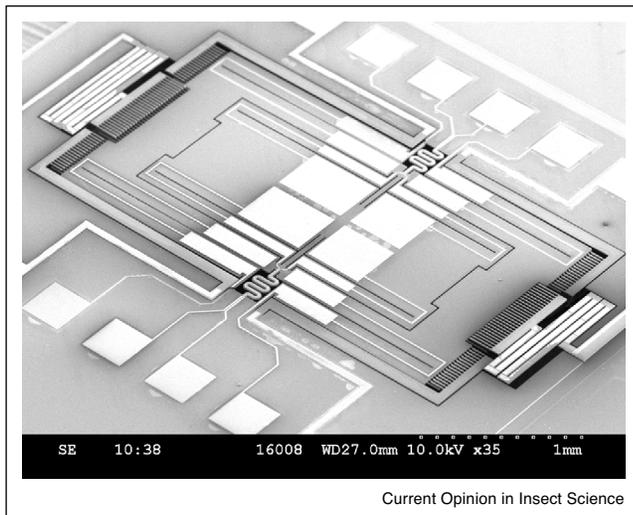

Ormia-inspired MEMS microphone with multiple working frequency bands operation, developed by Zhang *et al.* [62]. 29026

frequency operation [47^{*}]. The device has its best performance at 8 kHz, which is slightly below the first resonance and very similar to *Ormia*'s hearing organ (i.e. the best performance of *Ormia*'s ear occurs at 5 kHz, however the first resonance frequency is slightly higher than that value, which is around 7 kHz). At 8 kHz the slope of the mIPD versus the azimuth sound incident angle of this device is about 1.69 deg/deg.

The microphones presented here only permit the localization of sound on one axis, either the azimuth measured around the axis normal to the plane of the device, or the pitch, measured around the axis normal to the line between the two diaphragms. In any situation where either the azimuth or the pitch cannot be assumed to be zero there will be some ambiguity in the results, with the directional reading of the sensor describing a paraboloid surface in space. The problem could be potentially solved with an array of directional microphones [58,59]; however several teams have attempted to create sensors which extend the principles of *Ormia*-inspired hearing to two dimensions. The simplest of these consists of three mechanically linked diaphragms in a triangle formation around a central pivot [60^{*}]. Comparing the phase difference between any two diaphragms will yield a set of azimuth and pitch angles, which can then be correlated to the set produced by another pair of diaphragms to localize the sound source [61]. Although this sensor is capable of resolving the ambiguity in pitch and azimuth angle it does so by triangulation and offers little improvement over a similarly spaced array of *Ormia*-inspired microphones. In 2018 Zhang *et al.* introduced a further new microphone design. The design has two pairs of orthogonal

diaphragms, utilising the *Ormia* paradigm [62]. Each pair has independent directionality responses, leading to the potential for 3D sound localization. This single device can be regarded as two individual bi-directional microphones. It is also notable that this device combines both piezoelectric and capacitive sensing. Ono *et al.* [63,64] and Chen *et al.* [65] have proposed centrally supported gimbals to achieve the same goal, however, all these designs are either on the meso-scale or are proposed models only.

Second order Ormia inspired microphones

A second-order directional microphone has better ability to reject off-axis noise since it detects the sound location through estimating the second spatial derivative of the pressure gradient. The first model of second-order *Ormia*-inspired MEMS microphone was designed by Liu *et al.* [18,66], which joins two single *Ormia*-inspired first-order polysilicon microphones built by Miles *et al.* mentioned above with an S-type beam in the middle. Developing Liu's work, Albahri [67^{*}] optimized the model and replaced the S-type connection with a simple rectangular beam and added extra mass to the sides of the rotating plates to reduce the influence of any mismatch between the two single microphones. Meanwhile, Huo [68] changed the two diaphragms into a structure constructed with comb fingers, and removed the hinge. In theory, this gives the microphone a wide bandwidth of operation as the relative motion of the two diaphragms is not dependent on the frequency, however the sensitivity of the second order microphone increases with the square of the surface area, rather than being directly proportional, leading to significant miniaturisation challenges.

Conclusions

Biomimetic microphones, originally inspired by the mechanical structure of *O. ochracea*'s hearing organ, have higher directionality and are more suitable for micro-fabrication sensitivity than any conventional directional microphone array. They amplify the time delay and intensity difference efficiently between two membranes despite their tiny dimensions. Relying on different design concepts, such microphones can be made more complex in order to achieve higher mechanical sensitivity, or be simplified to decrease difficulties in fabrication. Designs can be divided into various groups, including first-order see-saw model and clamped diaphragms models, and second-order models. However, this model does require an omnidirectional microphone to get the sound pressure variation and bring full function to a system that requires accurate sound incident angle definition. The clamped-diaphragm model uses mIPD to locate sound and solve the omnidirectional microphone problem. But the fixed ends boundary of the diaphragm in this model generates a reaction force and so degrades the effective force driving vibration. The small displacement of the membranes can only be measured using optical (fibre) techniques so far. Despite patents relating to *O. ochracea* inspired

microphones now numbering in double figures and stretching back nearly 20 years, there is still research ongoing to solve the various issues to implementing these microphones in commercial, real-world applications. The growing market for miniature microphones, and need for technical improvements, across industries including mobile telecommunications, hearing prostheses and computing, suggests that such research efforts will continue into the future.

Conflict of interest statement

Nothing declared.

Acknowledgements

This work was supported by the EPSRC under grant EP/M026701/1 and by the European Research Council under the European Union's Seventh Framework Programme (FP/2007-2013)/ERC Grant Agreement n. [615030].

References and recommended reading

Papers of particular interest, published within the period of review, have been highlighted as

- of special interest
 - of outstanding interest
1. Gay SL, Benesty J: *Acoustic Signal Processing for Telecommunication*. US: Springer; 2001.
 2. Ianniello J: **Time delay estimation via cross-correlation in the presence of large estimation errors**. *IEEE Trans Acoust* 1982, **30**:998-1003.
 3. Popper A, Fay R: *Sound Source Localization*. Springer Science & Business Media; 2005.
 4. Gerzon MA: **Maximum directivity factor of *n*th-order transducers**. *J Acoust Soc Am* 1976, **60**:278-280.
 5. Yost WA, Gourevitch G: *Directional Hearing*. Springer-Verlag; 1987.
 6. Cade WH, Ciceran M, Murray A-M: **Temporal patterns of parasitoid fly (*Ormia ochracea*) attraction to field cricket song (*Gryllus integer*)**. *Can J Zool* 1996, **74**:393-395.
 7. Edgecomb RS, Robert D, Read MP, Hoy RR: **The tympanal hearing organ of a fly: phylogenetic analysis of its morphological origins**. *Cell Tissue Res* 1995, **282**:251-268.
 8. Miles RN, Robert D, Hoy RR: **Mechanically coupled ears for directional hearing in the parasitoid fly *Ormia ochracea***. *J Acoust Soc Am* 1995, **98**:3059-3070.
 9. Adamo SA, Robert D, Hoy RR: **Effects of a tachinid parasitoid, *Ormia ochracea*, on the behaviour and reproduction of its male and female field cricket hosts (*Gryllus* spp)**. *J Insect Physiol* 1995, **41**:269-277.
 10. Robert D, Amoroso J, Hoy RR: **The evolutionary convergence of hearing in a parasitoid fly and its cricket host**. *Science* 1992, **258**:1135-1137.
 11. Muller P, Robert D: **A shot in the dark: the silent quest of a free-flying phonotactic fly**. *J Exp Biol* 2001, **204**:1039-1052.
 12. Robert D, Miles RN, Hoy RR: **Tympanal mechanics in the parasitoid fly *Ormia ochracea*: intertympanal coupling during mechanical vibration**. *J Comp Physiol A Sens, Neural, Behav Physiol* 1998, **183**:443-452.
 13. Mason AC, Oshinsky ML, Hoy RR: **Hyperacute directional hearing in a microscale auditory system**. *Nature* 2001, **410**:686-690.
 14. Robert D, Miles RN, Hoy RR: **Directional hearing by mechanical coupling in the parasitoid fly *Ormia ochracea***. *J Comp Physiol A* 1996, **179**:29-44.
 15. Yu M: *Fly Ear Inspired Miniature Acoustic Sensors for Detection and Localization*. 2011.
 16. Lee J-H: **Biomimetic idealization of a mechanically coupled acoustic sound sensing mechanism**. *Simulation* 2017, **94**:131-143.
 17. Miles RN, Hoy RR: **The development of a biologically-inspired directional microphone for hearing aids**. *Audiol Neurotol* 2006, **11**:86-94.
 18. Miles RN, Liu Y, Su Q, Cui W: **A silicon directional microphone with second-order directivity**. *19th International Congress on Acoustics*. 2007:1-6.
 19. Gibbons C, Miles RN: **Design of a biomimetic directional microphone diaphragm**. *International Mechanical Engineering Congress and Exposition*. 2000:1-7.
 20. Miles RN, Gibbons C, Gao J, Yoo K, Su Q, Cui W: **A silicon nitride microphone diaphragm inspired by the ears of the parasitoid fly *Ormia ochracea***. *J Acoust Soc Am* 2001, **110**:2645.
 21. Mackie DJ, Jackson JC, Brown JG, Uttamchandani D, Windmill JFC: **Directional acoustic response of a silicon disc-based microelectromechanical systems structure**. *Micro Nano Lett* 2014, **9**:276-279 <http://dx.doi.org/10.1049/mnl.2013.0677>.
 22. An P, Yuan W, Ren S: **MEMS biomimetic acoustic pressure gradient sensitive structure for sound source localization**. *Sensors (Basel)* 2009, **9**:5637-5648.
 23. Gee DN, Liu HJ, Currano L, Yu M: **Enhanced directional sensitivity of a biomimetic MEMS acoustic localization sensor**. *Phononic Microdevices/Microstructures for Sensing II* 2010, **7682**:1-8.
 24. Liu H, Yu M: **Fly-Ear Inspired Miniature Acoustic Sensors**. *The 6th International Workshop on Advanced Smart Material and Smart Structures Technology*. 2011:1-8.
 25. Yu M, Liu H: **Biology-inspired miniature system and method for sensing and localizing acoustic signals**. 2013.
 26. Currano LJ, Liu H, Gee D, Yang B, Yu M: **Microscale implementation of a bio-inspired acoustic localization device**. *SPIE Bio-inspired/Biomimetic Sensor Technologies and Applications*. 2009. 73210B.
 27. Liu H, Chen Z, Yu M: **Biology-inspired acoustic sensors for sound source localization**. *SPIE Sensors and Smart Structures Technologies for Civil, Mechanical, and Aerospace Systems*. 2008. 69322Y.
 28. Yoo K, Gibbons C, Su QT, Miles RN, Tien NC: **Fabrication of biomimetic 3-D structured diaphragms**. *Sens Actuators A Phys* 2002, **97-98**:448-456.
 29. Tan L, Miles RN, Weinstein MG, Miller RA, Su Q, Cui W, Gao J: **Response of a biologically inspired MEMS differential microphone diaphragm**. *Proc. SPIE* 2002, **4743** <http://dx.doi.org/10.1117/12.448378> Unattended Ground Sensor Technologies and Applications IV, (7 August 2002).
 30. Cui W: *Analysis, Design and Fabrication of a Novel Silicon Microphone*. State University of New York at Binghamton; 2004.
 31. Cui W, Bicen B, Hall N, Jones SA, Degertekin FL, Miles RN: **Optical sensing in a directional MEMS microphone inspired by the ears of the parasitoid Fly, *Ormia Ochracea***. *19th IEEE International Conference on Micro Electro Mechanical Systems*. 2006:614-617.

32. Cui W, Miles RN, Su Q: **The design, fabrication and characterization of a novel miniature silicon microphone diaphragm.** *TechConnect Briefs* 2009, **1**:432-435.
33. Ishfaqe A, Kim B: **Analytical modeling of squeeze air film damping of biomimetic MEMS directional microphone.** *J Sound Vib* 2016, **375**:422-435.
34. Ishfaqe A, Kim B: **Design of Centrally Supported Biomimetic MEMS Microphone for Acoustic Source Localization.** *ASME ASME International Mechanical Engineering Congress and Exposition . Micro- and Nano-Systems Engineering and Packaging*; 2015 <http://dx.doi.org/10.1115/IMECE2015-51285>.
35. Ishfaqe A, Kim B: **Squeeze film damping analysis of biomimetic micromachined microphone for sound source localization.** *Sens Actuators A Phys* 2016, **250**:60-70.
36. Yoo K, Yeh J-LA, Tien NC, Gibbons C, Su Q, Cui W, Miles RN: **Fabrication of a biomimetic corrugated polysilicon diaphragm with attached single crystal silicon proof masses.** *Transducers' 01 Eurosensors XV.* Berlin, Heidelberg: Springer; 2001, 130-133.
37. Miles RN, Degertekin FL: Optical sensing in a directional MEMS microphone. 2010.
38. Bicen B, Jolly S, Jeelan K, Garcia CT, Hall NA, Degertekin FL, Su Q, Cui W, Miles RN: **Integrated optical displacement detection and electrostatic actuation for directional optical microphones with micromachined biomimetic diaphragms.** *IEEE Sens J* 2009, **9**:1933-1941.
- The authors gives an optical sensing solution consisting of a tiled vertical cavity surface emitting laser (VCSEL), a diffraction grating on the diaphragm and photodetectors for the see-saw like microphone.
39. Cui W, Miles RN, Su Q, Homentcovski D: **A bio-inspired miniature comb sense differential microphone diaphragm.** *Micro and Nano Systems . ASME. ASME International Mechanical Engineering Congress and Exposition*; 2010:143-148 <http://dx.doi.org/10.1115/IMECE2010-38179>.
- A more commonly used sensing method - capacitive comb sensing - is applied on a see-saw like Ormia-inspired microphone designed by Miles et al. expanding the application of their research.
40. Miles RN, Cui W, Su QT, Homentcovski D: **A MEMS low-noise sound pressure gradient microphone with capacitive sensing.** *J Microelectromechanical Syst* 2015, **24**:241-248.
41. Miles R: **Comparisons of the performance of commercially-available hearing aid microphones to that of the Binghamton Ormia-inspired gradient microphone.** *J Acoust Soc Am* 2017, **141**:3794.
- The author compares the see-saw like Ormia-inspired microphone with a commercial directional Knowles MEMS microphone and proves that the Ormia-inspired microphones provide better performance in frequency response, noise floor and directionality with complete experimental results.
42. Hall NA, Okandan M, Littrell R, Bicen B, Degertekin FL: **Micromachined optical microphone structures with low thermal-mechanical noise levels.** *J Acoust Soc Am* 2007, **122**:2031-2037.
43. Kuntzman ML, Gloria Lee J, Hewa-Kasakarage NN, Kim D, Hall NA: **Micromachined piezoelectric microphones with in-plane directivity.** *Appl Phys Lett* 2013, **102**:10-14.
44. Kuntzman ML, Hall NA: **Sound source localization inspired by the ears of the Ormia ochracea.** *Appl Phys Lett* 2014, **105**:033701.
45. Kuntzman ML, Hewa-Kasakarage NN, Rocha A, Kim D, Hall NA: **Micromachined in-plane pressure-gradient piezoelectric microphones.** *IEEE Sens J* 2015, **15**:1347-1357.
46. Reid A, Uttamchandani D, Windmill JFC: **Optimization of a bio-inspired sound localization sensor for high directional sensitivity.** *2015 IEEE Sensors.* 2015:1-4.
47. Liu H, Currano L, Gee D, Helms T, Yu M: **Understanding and mimicking the dual optimality of the fly ear.** *Sci Rep* 2013, **3**:1-6.
- A relatively integrated device is developed based on the concept described in Ref. [15••] is introduced.
48. Reid A, Windmill JFC, Uttamchandani D: **Bio-inspired sound localization sensor with high directional sensitivity.** *Procedia Eng* 2015, **120**:289-293.
- The directional sensitivity of a see-saw like microphone is enhanced via increasing the coupling strength based on the dual optimization concept mentioned in Ref. [15••].
49. Miles RN, Su Q, Cui W, Shetye M, Degertekin FL, Bicen B, Garcia C, Jones S, Hall N: **A low-noise differential microphone inspired by the ears of the parasitoid fly Ormia ochracea.** *J Acoust Soc Am* 2009, **125**:2013-2026.
50. Zhang Y, Bauer R, Whitmer WM, Brimijoin WO, Uttamchandani D, Windmill JFC, Jackson JC: **Development of a biologically inspired MEMS microphone.** *2017 IEEE Sensors.* 2017:1-3.
51. Zhang Y, Bauer R, Windmill JFC, Uttamchandani D: **Multi-band asymmetric piezoelectric MEMS microphone inspired by the Ormia ochracea.** *2016 IEEE 29th International Conference on Micro Electro Mechanical Systems (MEMS).* 2016:1114-1117.
52. Zhang Y, Windmill JFC, Uttamchandani D: **Biomimetic MEMS directional microphone structures for multi-band operation.** *2014 IEEE Sensors.* 2014:440-443.
53. Zhang Y, Bauer R, Windmill JF, Uttamchandani D, Jackson J: **New Ormia-inspired directional microelectromechanical systems microphone operating in a low-frequency band.** *J Acoust Soc Am* 2017, **141**:3794.
54. Bauer R, Zhang Y, Jackson JC, Whitmer WM, Brimijoin WO, Akeroyd MA, Uttamchandani D, Windmill JFC: **Influence of microphone housing on the directional response of piezoelectric MEMS microphones inspired by Ormia Ochracea.** *IEEE Sens J* 2017, **17**:5529-5536.
- In order to improve the acoustic sensitivity of the microphone operating below the ceiling of the audio range, three more resonance frequencies are added and evenly distributed across the frequency range of interest via introducing one more coaxial rotational plate into the see-saw like model. Moreover, the paper also discusses the impact of packaging on this kind of dual-plate microphone.
55. Zhang Y, Bauer R, Jackson JC, Whitmer WM, Windmill JFC, Uttamchandani D: **A low-frequency dual-band operational microphone mimicking the hearing property of Ormia Ochracea.** *J Microelectromechanical Syst* 2018, **27**:667-676.
- The design focuses on increasing acoustic frequency response at low-frequency range below 3 kHz to improve use for human speech recognition, and also embeds both piezoelectric and capacitive sensing units.
56. Liu HJ, Yu M, Currano L, Gee D: **Fly-ear inspired miniature directional microphones: modeling and experimental study.** *ASME 2009 International Engineering Congress.* 2009:1-7.
57. Liu H, Zhang X, Yu M: **Understanding fly-ear inspired directional microphones.** *Proc. SPIE 7292, Sensors and Smart Structures Technologies for Civil, Mechanical, and Aerospace Systems 2009* 2009 <http://dx.doi.org/10.1117/12.817703>. 72922M (30 March 2009).
58. Wilmott D, Alves F, Karunasiri G: **Bio-inspired miniature direction finding acoustic sensor.** *Sci Rep* 2016, **6**:1-8.
59. Xu H, Xu X, Jia H, Guan L, Bao M: **A biomimetic coupled circuit based microphone array for sound source localization.** *J Acoust Soc Am* 2015, **138**:EL270-EL275.
60. Lisiewski AP, Liu HJ, Yu M, Currano L, Gee D: **Fly-ear inspired micro-sensor for sound source localization in two dimensions.** *J Acoust Soc Am* 2011, **129**:EL166-EL171.
- The author illustrates a typical example of extending a 1D sound localization clamped-diaphragm biomimetic microphone to a 2D sound localization device.
61. Lu L, Sun H, Wu M, Cheng X, Yang J, Tian J: **Design and parameter study of a biologically inspired sound source locator.** *The 21st International Congress on Sound and Vibration.* 2014.
62. Zhang Y, Bauer R, Whitmer WM, Jackson JC, Windmill JFC, Uttamchandani D: **A MEMS microphone inspired by Ormia for spatial sound detection.** *2018 IEEE Micro Electro Mechanical Systems (MEMS).* 2018:253-256.

63. Ono N, Saito A, Ando S: **Bio-mimicry sound source localization with gimbals diaphragm**. *IEEJ Trans Sens Micromach* 2003, **123**:92-97.
64. Ono N, Saito A, Ando S: **Design and experiments of bio-mimicry sound source localization sensor with gimbals-supported circular diaphragm**. *TRANSDUCERS' 03. 12th International Conference on Solid-State Sensors, Actuators and Microsystems*. 2003:935-938.
65. Chen C-C, Y-T Cheng: **Physical analysis of a biomimetic microphone with a central-supported (C-S) circular diaphragm for sound source localization**. *IEEE Sens J* 2011, **12**:1504-1512.
66. Miles R: High-order directional microphone diaphragm. 2005, 1.
67. Albahri S: *Design and development of second order MEMS sound pressure gradient sensor*. 2011.
The dissertation provides the clear theoretical basis and design details of the second-order *Ormia*-inspired MEMS microphone.
68. Huo X: *Design, analysis and characterization of a miniature second-order directional microphone*. 2009.